

EU-TYPE EXAMINATION CERTIFICATE

Qingdao Comcore Technologies Co., Ltd.
8 Floor, Block A, International Innovation Park, No.1
Keyuanweiyi Rd, Laoshan District, 266061, Qingdao
China

EU-Type Examination
Certificate No.
103680205-25

Revision 0



Type TA15
Object Electronic single-phase two-wire two-element energy meter.
Direct connected.

The object has been assessed and meets the requirements of

EU Directive 2014/32/EU
Module B

The energy meter(s) meet(s) the essential requirements of Annex V of EU Directive 2014/32/EU, on the harmonization of the laws of Member States relating to the making available on the market of measuring instruments (recast).

This Certification is based on the report(s) listed in the report list in this Certificate.

This Certificate is valid until: March 14, 2035.

This Certificate comprises 8 pages in total.

Issued by KEMA B.V.
Klingelbeekseweg 195,
Arnhem, The Netherlands
Notified Body 2290


Marten Dekker
Operations Director Netherlands

Arnhem, March 14, 2025



REVISION OVERVIEW

The edition with the highest revision number always replaces the earlier issued editions.

Rev. No.	Date of issue	Reason
0	March 14, 2025	First issue

REPORT LIST


This Certificate is issued based on the following reports.

Report number	Revision	Firmware version
103680201-25	0	TA19KV0112PLTG24042601
103680202-25	0	TA19KV0112PLTG24042601
103680203-25	0	TA19KV0112PLTG24042601

1 TECHNICAL DATA

Manufacturer	Qingdao Comcore Technologies Co., Ltd. 8 Floor, Block A, International Innovation Park, No.1 Keyuanweiyi Rd,Laoshan District, Qingdao, 266061, China
Production location	Qingdao Comcore Technologies Co., Ltd. 8 Floor, Block A, International Innovation Park, No.1 Keyuanweiyi Rd,Laoshan District, Qingdao, 266061, China
Type	TA15
Model	-
Connection	Direct
Type of circuit	1P2W, two-element
Accuracy class Wh	1/B
Accuracy class varh	2
Meter constant	1000 imp/kWh 1000 imp/kvarh
V range	220 – 240 V
I range I_{min} - I_n (I_{max})	0,25 - 5(80)A
Frequency	50 Hz
Temperature range	-40 .. 70 °C
Use	Indoor
IP rating	IP54
Protection Class	II
Impulse voltage	6 kV
Internal clock	Crystal controlled
Environmental class	M1, M2, E1 and E2, CISPR32 class B
Utilisation category	UC2
Token interface	Keypad interface
Payment type	kWh
LR Firmware ID	TA19KV0112PLTG24042601
LR Firmware CRC	05C1457C
Register	LCD
Registry method	bi-directional method with separate registers: received- and delivered energy is added in separate registers. At received and delivered energy the amount of energy is deducted from the remain energy.

2 PHOTOGRAPHS AND SEALING

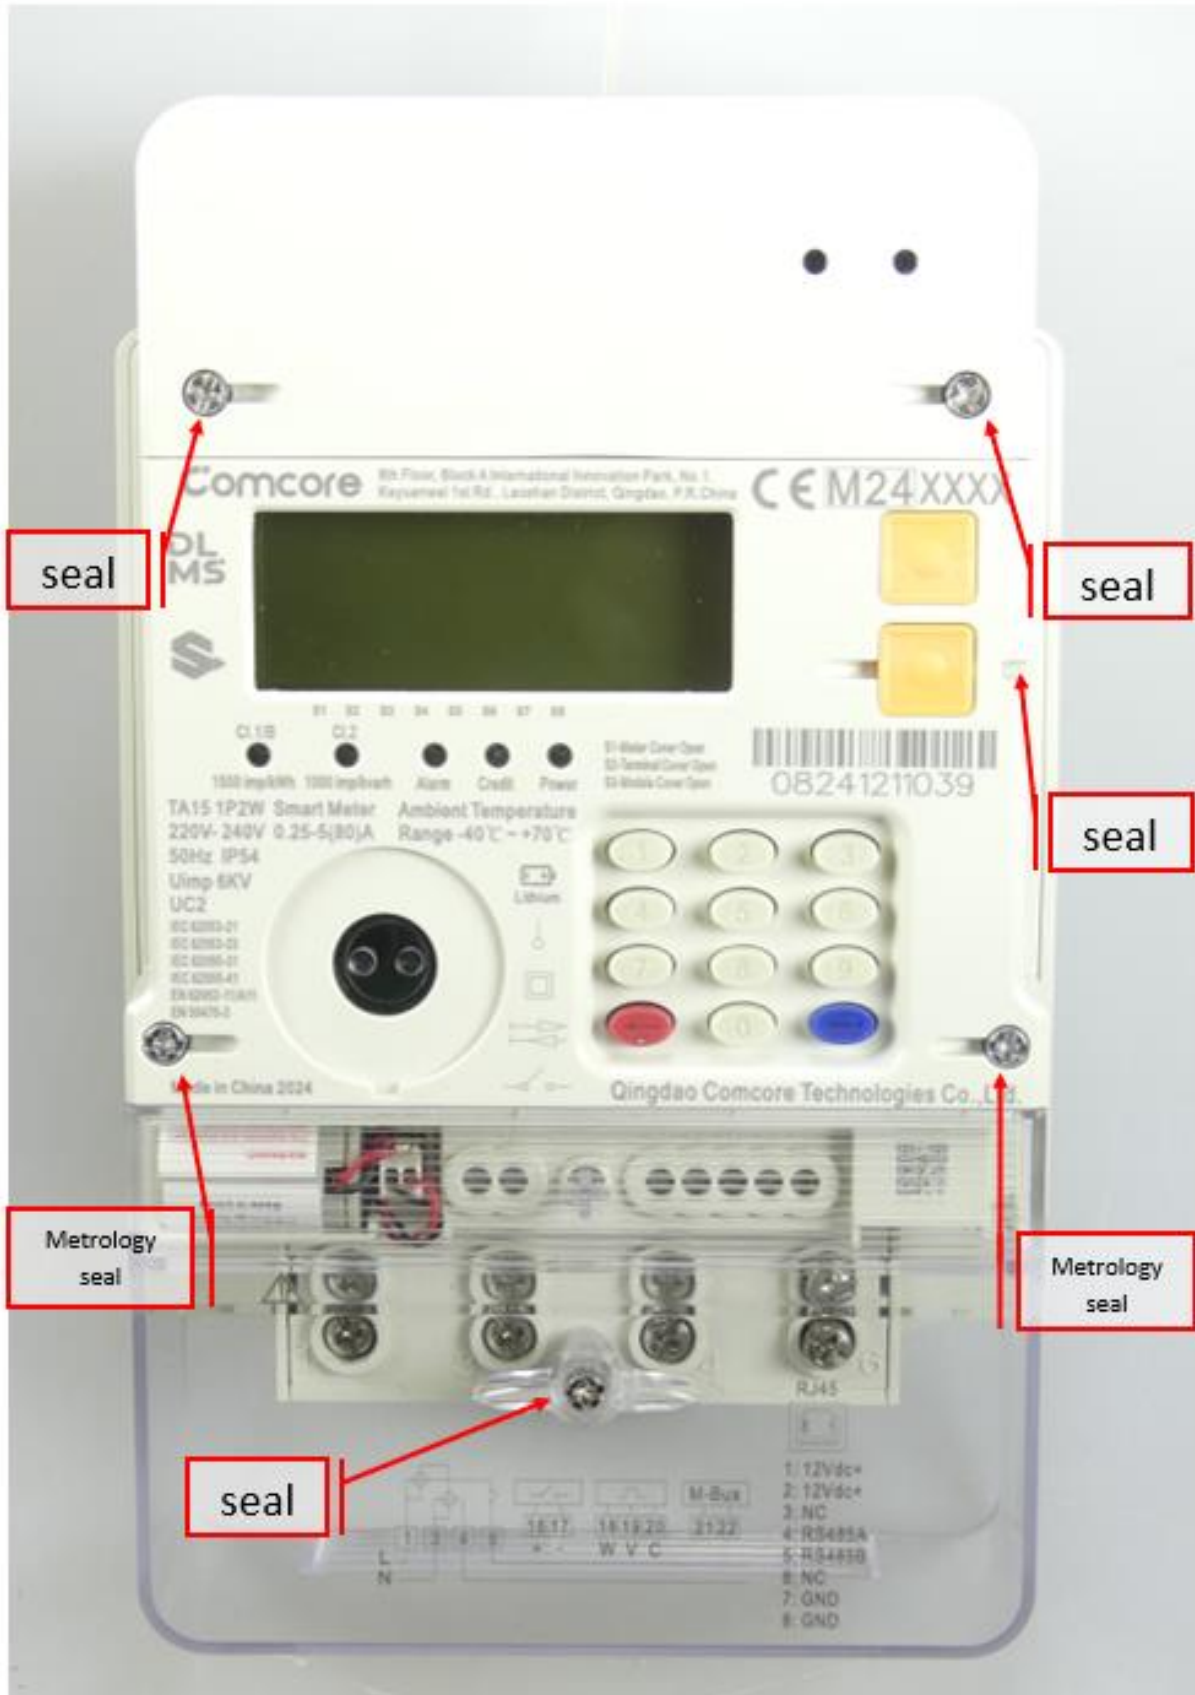

3 EXAMPLES OF NAME PLATES



4 CALCULATION OF THE COMPOSITE ERROR / MPE

During the type approval test the intrinsic errors for temperature, voltage and frequency variation are determined per load point. The composite error is determined with the following formula:

$$\varepsilon_m = \sqrt{\varepsilon^2(I, \cos\varphi) + \delta^2(T, I, \cos\varphi) + \delta^2(U, I, \cos\varphi) + \delta^2(f, I, \cos\varphi)}$$

Where

$\varepsilon^2(I, \cos\varphi)$ = Intrinsic error of the meter at a certain load

$\delta^2(T, I, \cos\varphi)$ = Additional error due to the variation of the temperature at the same load

$\delta^2(U, I, \cos\varphi)$ = Additional error due to the variation of the voltage at the same load

$\delta^2(f, I, \cos\varphi)$ = Additional error due to the variation of the frequency at the same load

Results are in the table below:

Serial number:		08240507023							
		Wh, 220 V, 0,25-5(80) A, 50 Hz, in L							
		Composite error							
Current	cosφ	-40°C	-25°C	-10°C	5°C	30°C	40°C	55°C	70°C
I_{min}	1	0,39%	0,27%	0,20%	0,14%	0,12%	0,13%	0,15%	0,18%
I_{tr}	1	0,37%	0,25%	0,18%	0,11%	0,08%	0,09%	0,16%	0,16%
I_{tr}	0,5i	0,34%	0,25%	0,18%	0,13%	0,12%	0,15%	0,19%	0,18%
I_{tr}	0,8c	0,36%	0,24%	0,17%	0,11%	0,09%	0,11%	0,15%	0,19%
I_n	1	0,35%	0,24%	0,16%	0,08%	0,03%	0,07%	0,12%	0,15%
I_n	0,5i	0,35%	0,25%	0,16%	0,08%	0,03%	0,06%	0,11%	0,14%
I_n	0,8c	0,35%	0,24%	0,15%	0,08%	0,05%	0,08%	0,13%	0,15%
I_{max}	1	0,12%	0,09%	0,07%	0,05%	0,04%	0,05%	0,06%	0,06%
I_{max}	0,5i	0,08%	0,07%	0,07%	0,07%	0,07%	0,07%	0,08%	0,07%
I_{max}	0,8c	0,09%	0,08%	0,07%	0,07%	0,07%	0,07%	0,07%	0,07%
Requirements									
Any	1	4,00%	3,50%	2,50%	2,00%	2,00%	2,50%	3,50%	4,00%
Any	0,5/0,8	4,00%	3,50%	2,50%	2,00%	2,00%	2,50%	3,50%	4,00%

5 OPTIONS AND VARIANTS

Overview of variants with details

Type designation	Details of the meter
TA15	<ul style="list-style-type: none">• Communication options:<ul style="list-style-type: none">optical portRS485M-BusPulse output• Supply control switch• External valve control• neutral Measurement

END OF DOCUMENT

The laboratories of KEMA Labs are:

- CESI S.p.A., Milan, Italy, accredited by ACCREDIA in accordance with ISO/IEC 17025:2017 under no. 0030L.
- FGH Engineering & Test GmbH, Mannheim, Germany, accredited by DAkKS in accordance with DIN EN ISO/IEC 17025:2018 under no. D-PL-12110-01-00.
- IPH Institut "Prüffeld für elektrische Hochleistungstechnik" GmbH, Berlin, Germany accredited by DAkKS in accordance with DIN EN ISO/IEC 17025:2018 under nos. D-PL-12107-01-00 and D-K-12107-01-00.
- KEMA B.V., Arnhem, The Netherlands, accredited by RvA in accordance with EN ISO/IEC 17025:2017 under nos. L020, L218 and K006 and with EN ISO/IEC 17065:2012 under no. C685.
- KEMA Labs, Zkušebnictví, a.s., Prague, the Czech Republic, testing laboratory no. 1035 accredited by CAI in accordance with ČSN EN ISO/IEC 17025:2018.
- KEMA-Powertest, LLC, Chalfont, United States, accredited by A2LA in accordance with ISO/IEC 17025:2017 under no. 0553.01.

Tests are carried out under the scope of accreditation, unless otherwise indicated in the chapter 'Tests carried out'.